

Selecting Reagents for Multicolor Flow Cytometry

From HotLines Platinum Edition, Fall 2006

By Holden Maecker and Joe Trotter



The availability of flow cytometers capable of detecting 6, 8, or more colors has spurred the discovery of new fluorochromes and the development of antibody conjugates. However, the complexities of choosing antibody combinations are such that simply using a random combination of fluorochromes for a particular set of antibody specificities is unlikely to provide optimal results. On the other hand, with a bit of forethought, one can usually avoid many rounds of trial and error. The goal of this article is to provide some simple guidelines to aid in the selection of reagent panels for multicolor flow cytometry, which should result in more successes than failures.

The basics: Know your instrument

Reagent selection starts with your instrument configuration. The lasers and detectors that you have available dictate whether or not you can excite a given fluorochrome, and whether or not you have enough detectors to read out a given combination of fluorochromes. The design of the optical system also impacts the efficiency with which particular dyes are detected, as do the instrument settings, including PMT voltages (see the BD Application Note, *Establishing Optimum Baseline PMT Gains to Maximize Resolution on BD Biosciences Digital Flow Cytometers* at bdbiosciences.com/baselineoptimization). Finally, the choice of optical filters that are used with each detector greatly influences the brightness of one fluorochrome versus another. One can think of filter selection as a give-and-take process: using a wider bandpass filter can increase the ability to detect a given fluorochrome, but may also increase the amount of spillover detected in that detector from other neighboring fluorochromes. A good way to visualize these effects is by virtual testing of filter combinations using a web tool such as the fluorescence spectrum viewer at bdbiosciences.com/spectra. Here you can get an idea of predicted spillovers* for particular fluorochromes and filter combinations.

Fluorochromes: Go for the bright

Given the many differences in instrument configuration, it is impossible to universally state the “best” fluorochromes to use in combinations of 6, 8, or more colors. However, if one considers a particular cytometer such as the BD™ LSR II instrument, it is possible to rank available dyes according to their brightness on that instrument (when configured with a specified set of lasers and filters). But how exactly do we define and measure brightness? A good definition of brightness should probably start with *resolution sensitivity*, the ability to discriminate a dim positive signal from background. Background in a particular detector is influenced by electronic noise, cell autofluorescence, and spillover from other detectors. To the extent that these factors introduce noise, they also increase the width (or standard deviation, SD) of a negative fluorescence peak (see **Figure 1**). As such, a good measure of resolution sensitivity is the stain index,¹ defined as D/W , where D is the difference between means of a positive and negative peak, and W is equal to 2 SD of the negative peak.

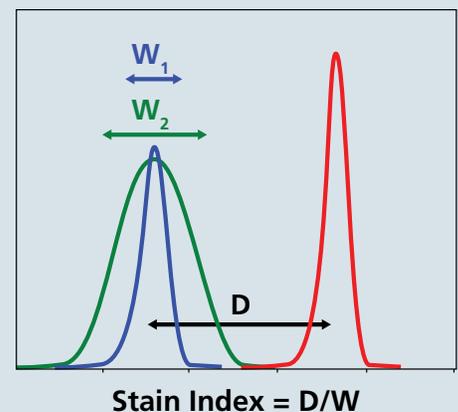


Figure 1. Resolution sensitivity (the ability to resolve a dim positive signal from background) depends upon the difference between positive and background peak means (D) and the spread of the background peak (W). The stain index is a metric that captures both of these factors.

* The predicted spillovers are normalized percentages of omitted fluorescence, and may not necessarily correspond to the percentage used for compensation due to the effects of varying detector gains.

Selecting Reagents for Multicolor Flow Cytometry (continued)

Table 1. Stain index of various fluorochrome conjugates on a BD LSR II flow cytometer.

Reagent	Clone	Filter	Stain Index
PE	RPA-T4	585/40	356.3
Alexa Fluor® 647 ¹	RPA-T4	660/20	313.1
APC ¹	RPA-T4	660/20	279.2
PE-Cy7 TM	RPA-T4	780/60	278.5
PE-Cy5 ²	RPA-T4	695/40	222.1
PerCP-Cy5.5 ²	Leu-3a	695/40	92.7
PE-Alexa Fluor® 610	RPA-T4	610/20	80.4
Alexa Fluor® 488 ³	RPA-T4	530/30	75.4
FITC ³	RPA-T4	530/30	68.9
PerCP ²	Leu-3a	695/40	64.4
APC-Cy7	RPA-T4	780/60	42.2
Alexa Fluor® 700	RPA-T4	720/45	39.9
Pacific Blue TM	RPA-T4	440/40	22.5
AmCyan	RPA-T4	525/50	20.2

^{1,2,3} Fluorochromes listed with the same superscript number are read in the same detector, and thus would not normally be used in combination.

When the same antibody is conjugated to various dyes, one can compare the stain index for those conjugates to get an idea of the relative brightness of the dyes on a particular instrument. This assumes, of course, that the conjugation chemistries for all of the reagents have been optimized. With this as a caveat, **Table 1** shows the stain index for a number of different CD4 conjugates, using the specified filters on a standard BD LSR II flow cytometer.

From this table, one can get an idea of the relative brightness of different fluorochromes on this platform. This leads to the first rule of reagent selection, which is to pick the brightest available fluorochromes. Suppose you have a 4-color panel consisting of reagents in FITC, PE, PerCP-Cy5.5, and APC, and you want to add a fifth color. PE-Cy7 is an obvious choice, since it is the brightest fluorochrome not already in your panel.

Minimize spillover

But brightness, on its own, only goes so far. The stain indexes listed in **Table 1** are calculated with the reagents run on their own, not as part of a cocktail. As soon as other reagents are added, spectral overlap (spillover) becomes an issue. Simply stated, the more colors one attempts to resolve, the more spillover between those colors that will have to be dealt with. We deal with spillover by applying compensation, which results in a correction being applied to all signals such that a cell population fluorescing only in PE, for example, will show no FITC fluorescence, on average. But while this is true for the population on average, individual cells will fall above or below the mean, and this data spread is higher when spectral overlap introduces additional noise.¹ Compensation, unfortunately, does not remove this noise. The effect of data spread is thus to reduce the resolution sensitivity, and therefore the stain index, for a

Table 2. Common choices for 6, 8, and 10-color experiments.

6-color	8-color	10-color
FITC or Alexa Fluor® 488	FITC or Alexa Fluor® 488	FITC or Alexa Fluor® 488
PE	PE	PE
–	–	PE-Texas Red® or PE-Alexa Fluor® 610
PerCP-Cy5.5	PerCP-Cy5.5	PerCP-Cy5.5
PE-Cy7	PE-Cy7	PE-Cy7
APC or Alexa Fluor® 647	APC or Alexa Fluor® 647	APC or Alexa Fluor® 647
–	–	Alexa Fluor® 680 or 700
APC-Cy7	APC-Cy7	APC-Cy7
–	AmCyan	AmCyan
–	Pacific Blue TM	Pacific Blue TM

fluorescence detector that receives spillover from other detector(s). As a result, we can state a second rule of reagent selection, which is to minimize the potential for spectral overlap when choosing a reagent combination. This can be in conflict with the first rule, which was to choose the brightest fluorochromes. For example, PE-Cy5 is very bright with regard to stain index (**Table 1**), but it has considerable spillover into the APC detector. While these two fluorochromes can be used together, the resolution sensitivity in APC will be reduced compared to, for example, a combination of PerCP-Cy5.5 and APC. This is a case where one might wish to sacrifice a certain amount of brightness in one detector to avoid spillover (and loss of resolution sensitivity) in another.

Colors and specificities: Define winning combinations

Taking the two rules above into account, one can generalize a set of fluorochromes that are reasonable choices to use for experiments requiring 6, 8, or more colors (**Table 2**). Note that these choices are based upon BD instruments (BD LSR II, BD FACSAriaTM cell sorter, or BD FACSCantoTM flow cytometer), and upon reagents that can be generally purchased as catalog antibody conjugates.

Once the fluorochromes to be used have been defined, one can begin to match antibody specificities to particular fluorochromes. In other words, one can select the actual conjugates to be used. For this purpose, brightness and spillover remain key issues, as the following example illustrates.

Imagine that you want to look at CD62L staining on CD8⁺ T cells. While CD8 is an abundant protein, and antibodies to it stain cells very brightly, CD62L is relatively dim (the protein is not abundant on the cell surface, and/or the available antibodies are of low affinity). Initially, one would be tempted to use the brightest available fluorochrome, PE, for CD62L, while using a dimmer fluorochrome, like FITC, for CD8. But FITC has considerable spillover into the PE

Selecting Reagents for Multicolor Flow Cytometry (continued)

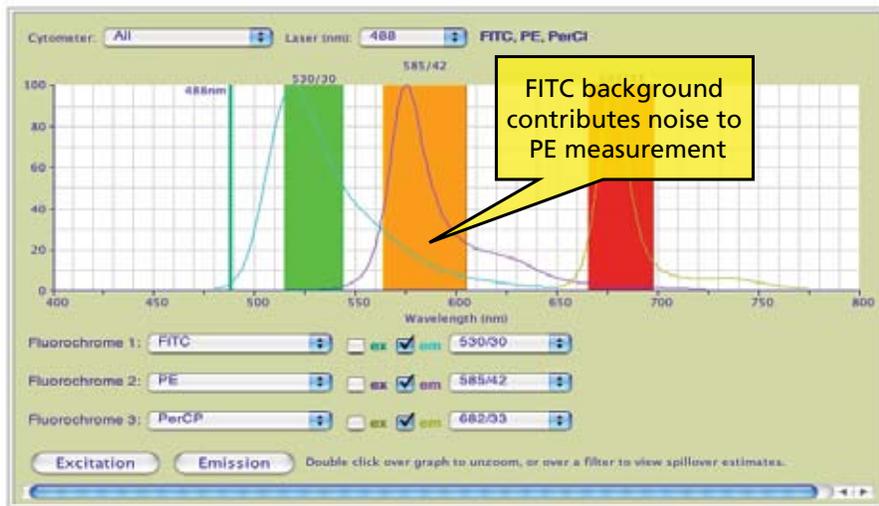


Figure 2. Spectral overlap of FITC into the PE detector. Taken from bdbiosciences.com/spectra.

detector (see **Figure 2**). The result is that, for CD8⁺ cells that are highly stained in the FITC detector, resolution sensitivity in PE is compromised, to the point that CD62L resolution may be suboptimal. There are multiple possible solutions to improve this, including:

1. Moving CD8 to a detector that has less spectral overlap with PE (like PerCP-Cy5.5 or APC).
2. Moving CD62L to a detector that is still relatively bright, but does not overlap with FITC (like APC or PE-Cy5). Note that in this example, only the CD8⁺ cells are highly stained in the FITC detector, so only CD8⁺ cells contribute to data spread in the PE detector. If one were interested in CD62L staining only on CD4⁺ (CD8⁻) cells, the original reagent combination (CD8 FITC, CD62L PE) would be fine.

This example illustrates two additional rules in reagent selection: Reserve the brightest fluorochromes for dim antibodies, and vice versa, but avoid spillover from bright cell populations into detectors requiring high sensitivity for those populations.

Tandem dyes: Watch out for degradation

One final topic to consider is the potential for tandem dye degradation. APC-Cy7, and to a lesser extent, PE-Cy7, can degrade in the presence of light, fixation, and elevated

temperatures so that they emit in the parent dye detector (APC or PE). This process often starts with a small subpopulation of cells, leading to false positive events in APC or PE.¹ By minimizing the exposure of samples to light, heat, and formaldehyde-based fixatives, this problem can be largely avoided. Still, for some applications, it may be desirable to think about an additional rule: consider the consequences of degradation of tandem dyes and whether this will compromise sensitive readouts in the APC or PE detectors. If so, a different reagent configuration may be in order. For situations in which final fixation of samples is required (eg, biohazardous samples), there is a stabilizing fixative available that helps prevent degradation of APC-Cy7 while still fixing cells (BD Biosciences **Cat. No. 338036**).

Controls to validate your panel

Once all of these considerations have been taken into account, you are ready to test a multicolor reagent cocktail. In so doing, there are two types of controls that you may wish to include in your initial testing: fidelity controls and fluorescence-minus-one (FMO) controls.² Fidelity controls are those that use a given antibody by itself (or with minimal additional gating reagents), and compare the results to the use of that antibody in a complete cocktail. From this, one can see the effect of additional reagents on the readout of

interest, to be sure that the other reagents are not compromising that readout. FMO controls are those that combine all the reagents in a given cocktail, except for one reagent of interest. These are useful to gauge the sensitivity of particular detectors in the context of the other reagents. They may also be used for routine gating of those detectors for which other means of setting gates are not possible or practical. In general, though, once a reagent panel has been well validated, it is not necessary to run all of these controls on a day-to-day basis.

To summarize, this article has set forth rules for selecting reagents for multicolor flow cytometry. These rules, although sometimes in conflict with each other, need to be balanced to achieve the best possible results:

- Rule 1:** Choose the brightest set of fluorochromes for your particular instrument configuration.
- Rule 2:** Choose fluorochromes so as to minimize the potential for spectral overlap.
- Rule 3:** Reserve the brightest fluorochromes for dim antibodies, and vice versa.
- Rule 4:** Avoid spillover from bright cell populations into detectors requiring high sensitivity for those populations.
- Rule 5:** Take steps to avoid tandem dye degradation, and consider its impact on the results.

With time, proven panels of multicolor reagents will become available, both in the literature and from manufacturers, such that many users will not have to start from scratch in designing reagent panels. Nevertheless, given the huge variety of applications of multicolor flow cytometry, most researchers will at least sometimes find themselves having to select their own multicolor reagents, we hope that these rules will prove helpful.

References

1. Maecker HT, Frey T, Nomura LE, and Trotter J. Selecting fluorochrome conjugates for maximum sensitivity. *Cytometry A*. 2004;62:169.
2. Baumgarth N and Roederer M. A practical approach to multicolor flow cytometry for immunophenotyping. *J. Immunol. Methods*. 2000;243:77.

Fluorochromes for combinations beyond the typical 5-color experiment

Multicolor Flow Cytometry Reagents

Expand your multicolor flow with options beyond the typical 5 colors

- BD Biosciences continues to increase our portfolio of multi-color reagents to support your cutting-edge research using the expanded fluorescence detection capabilities of our flow cytometers.
- We offer directly conjugated antibodies to fluorochromes that go beyond your typical 5 colors by providing colors off the violet, red, and blue lasers. These include AmCyan, Pacific Blue™, Alexa Fluor® 700, and PE-Cy7 conjugates to support up to 9-color staining with off-the-shelf reagents. See **page 5** for details.
- BD Biosciences Custom Conjugation Program* offers even more choices for your multicolor experiment design. This program offers multiple colors, as shown in the table below.

Custom conjugates available from BD Biosciences

Fluorochrome	Ex Max (nm)
Alexa Fluor® 405	401
Alexa Fluor® 488	495
Alexa Fluor® 594	590
Alexa Fluor® 647	650
Alexa Fluor® 680	679
Alexa Fluor® 700	696
AmCyan	457
APC	650
APC-Cy7	650
FITC	494
Pacific Blue™	405
PE-Cy5	496, 564
PE-Cy7	496, 564
PerCP	482
PerCP-Cy5.5	482
PE-Texas Red®	496, 564
Texas Red®	595

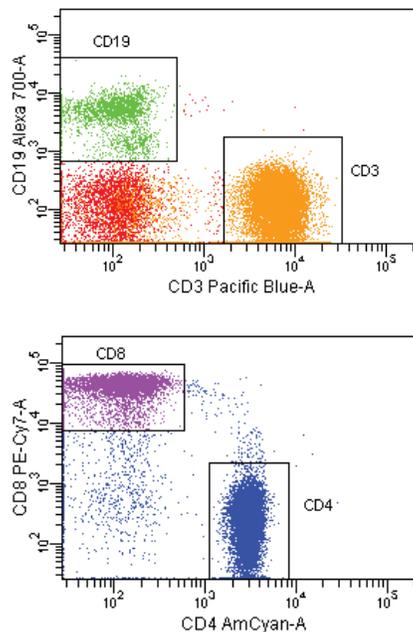


Figure 3. Example of the use of gating reagents (CD3, CD4, and CD19) using non-traditional fluorochrome conjugates excited by blue, red, and violet lasers.

Visit bdbiosciences.com/colors for details about our multicolor flow cytometry reagents.

*Please contact the Technical Service Department for more information about the Custom Conjugation Program.

Fluorochromes for combinations beyond the typical 5-color experiment *(continued)*

Name	Reactivity	Blue laser (488 nm)	Red laser (633 nm)	Violet laser (407 nm)	
		PE-Cy7 Ex Max (nm): 496, 564	Alexa Fluor® 700 Ex Max (nm): 696	Pacific Blue™ Ex Max (nm): 405	AmCyan Ex Max (nm): 457
CCR4	Hu	557864			
CCR6	Hu	557993			
CCR7	Hu	557648			
CD2	Hu	335786			
CD3	Hu	557851, 341091	557943	558117	339186
CD3	Bab, Cyno, Rhe	557749	557917	558124	
CD3e	Ms	552774		558214	
CD4	Hu	557852, 348789	557922	558116	339187
CD4	Ms	552775	557956	558107	
CD5	Hu	348790			
CD8	Hu	557746, 335787	557945	558207	339188
CD8	Bab, Cyno, Rhe	557750			
CD8a	Ms	552877	557959	558106	
CD10	Hu	341092			
CD11a	Ms	558191			
CD11b	Hu	557743		558123	
CD11b	Ms	552850	557960		
CD13	Hu	338425			
CD14	Hu	557742	557923	558121	
CD16	Hu	557744, 335788	557920	558122	
CD19	Ms	552854	557958		
CD19	Hu	557835, 341093	557921		339190
CD20	Hu	335793			
CD25	Hu	557741			
CD25	Ms	557744, 335789			
CD33	Hu	333946			
CD34	Hu	348791			
CD38	Hu	335790			
CD45	Hu	557748			339192
CD45	Ms	552848			
CD45R/B220	Ms	552772	557957	558108	
CD45RA	Hu	337167			
CD45RO	Hu	337168			
CD56	Hu	557747, 335791	557919		
CD69	Hu	557745			
CD69	Ms	552879			
CD95	Ms	557653			
CD117	Hu	339195			
CD195	Hu	557752			
CD274	Hu	558017			
HLA-DR	Hu	335795			
IFN-γ	Hu	557844, 557643			
IFN-γ	Ms	557649			
IgG ₁ , κ	Hu	348788			339185
IgG ₁ , κ	Ham	552811			
IgG ₁ , κ	Ms	557646, 557872	557882	558120	
IgG ₁ , κ	Rat	557645			
IgG ₁ , λ	Ham	557798			
IgG ₁ , λ	Rat	552869			
IgG _{2a} , λ	Ham	557652			
IgG _{2a} , κ	Rat	552784	557963	558109	
IgG _{2a} , κ (specific for TNP)	Ms	552868		558118	
IgG _{2b} , κ	Rat	552849			
IgM	Ms	552867			
IL-4	Hu	557989			
Ly-6G and Ly-6C	Ms	552985	557979		
NK-1.1	Ms	552878			
PD-1	Hu	558016			
PD-L1	Hu	558017			
TNF	Hu	557647			
TNF	Ms	557644			

Patents: PerCP: US 4,876,190; APC-Cy7: US 5,714,386

Selecting Reagents for Multicolor Flow Cytometry

**For ordering information and technical services
please contact your local BD Biosciences office.**

United States

Tel 877.232.8995
Fax 800.325.9637

Canada

Tel 888.259.0187
Fax 888.229.9918

Europe

Tel 32.53.720.550
Fax 32.53.720.549

Japan

Tel 0120.8555.90
Fax 81.24.593.5761

Asia Pacific

Tel 65.6861.0633
Fax 65.6860.1593

Latin America/Caribbean

Tel 55.11.5185.9645
Fax 55.11.5185.9895

For country-specific contact information,
visit bdbiosciences.com/how_to_order/international_offices.shtml

Pacific Blue™ is a trademark, and Alexa Fluor®, Cascade Blue®, and Texas Red® are registered trademarks of Molecular Probes, Inc.

The Alexa Fluor®, Pacific Blue™, and Cascade Blue® dye antibody conjugates in this product are sold under license from Molecular Probes, Inc. for research use only, excluding use in combination with microarrays, or as analyte specific reagents. The Alexa Fluor® dyes (except for Alexa Fluor® 430), Pacific Blue™ dye, and Cascade Blue® dye are covered by pending and issued patents.

Cy™ is a trademark of Amersham Biosciences Corp. Cy™ dyes are subject to proprietary rights of Amersham Biosciences Corp and Carnegie Mellon University and are made and sold under license from Amersham Biosciences Corp only for research and in vitro diagnostic use. Any other use requires a commercial sublicense from Amersham Biosciences Corp, 800 Centennial Avenue, Piscataway, NJ 08855-1327, USA.

BD flow cytometers are Class I (1) laser products. For Research Use Only. Not for use in diagnostic or therapeutic procedures. Not for resale. All applications are either tested in-house or reported in the literature. See Technical Data Sheets for details. © 2007 Becton, Dickinson and Company. All rights reserved. No part of this publication may be reproduced, transmitted, transcribed, stored in retrieval systems, or translated into any language or computer language, in any form or by any means: electronic, mechanical, magnetic, optical, chemical, manual, or otherwise, without prior written permission from BD Biosciences. Purchase does not include or carry any right to resell or transfer this product either as a stand-alone product or as a component of another product. Any use of this product other than the permitted use without the express written authorization of Becton, Dickinson and Company is strictly prohibited. Prices are subject to change without notice.

Shop online at shop.bdbiosciences.com



BD Biosciences
2350 Qume Drive
San Jose, CA 95131
bdbiosciences.com